



Step by step instructions

LAC 142 / LAC 342 / GLU 142 / CHO 142 / TRI 142

Single measurement

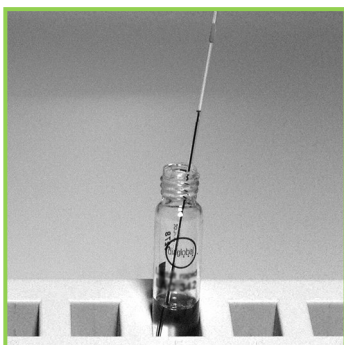


1. Insert capillary with 10 μ L sample into cuvette

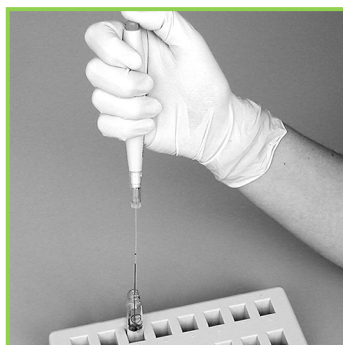


2. Eject sample several times with micropipetter into cuvette



3. Screw cap on
Turn cuvette upside down several times

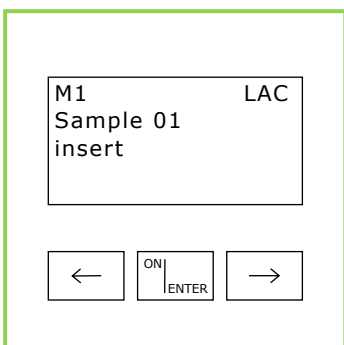

4. Switch photometer on with ON/ENTER key
Wait for device check, confirm with ON/ENTER
Select the required test, confirm with ON/ENTER

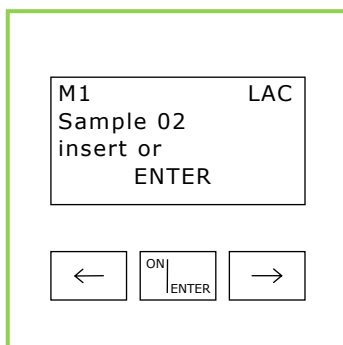


5. Zero point adjustment: Insert cuvette with sample (Fig. 3) into photometer, zero point is stored in memory
Remove cuvette after signal tone



6. Replace screw cap with starter cap



7. Turn cuvette upside down several times

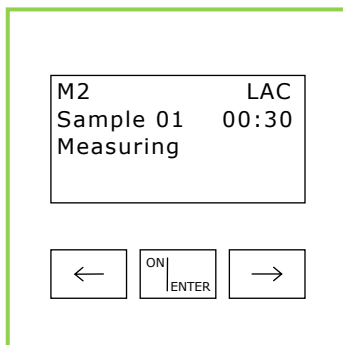

8. First press ON/ENTER
Then insert cuvette into photometer




9. Time is displayed, wait for measured value

Step by step instructions

LAC 142 / CHO 142 / TRI 142


Number of samples per series: Up to 20 samples at the same time

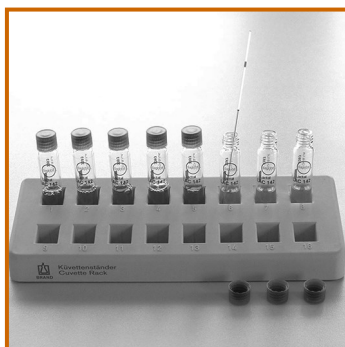


1. Eject all samples one after the other several times with micropipetter into cuvette



2. Screw all caps on again
Turn cuvettes upside down several times

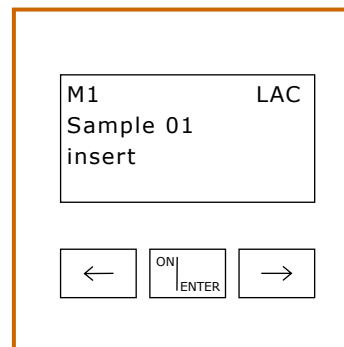

3. Switch photometer on with ON/ENTER key
Wait for device check, confirm with ON/ENTER
Select the required test, confirm with ON/ENTER

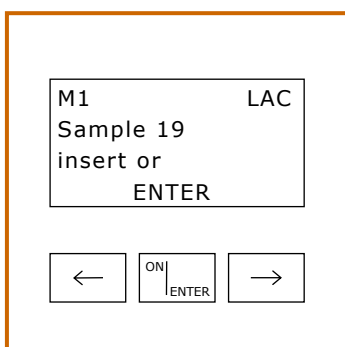


4. Zero point adjustment: Insert cuvettes with samples (Fig. 2) one after the other into photometer, all zero points are stored in memory


Note: Ensure the correct order of the samples!



5. After the zero point adjustment of the last cuvette replace all screw caps with starter caps

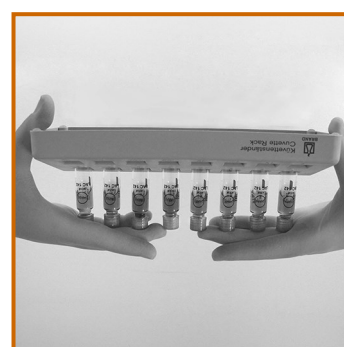


6. Turn all cuvettes **simultaneously** upside down, repeat several times

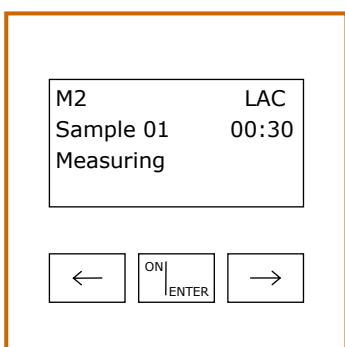

7. First press ON/ENTER key
Then insert 1st cuvette into photometer
Time is displayed, wait for measured value



8. Read the measured value of the 1st cuvette, remove cuvette
Insert 2nd cuvette, read the measured value, remove cuvette, and so on

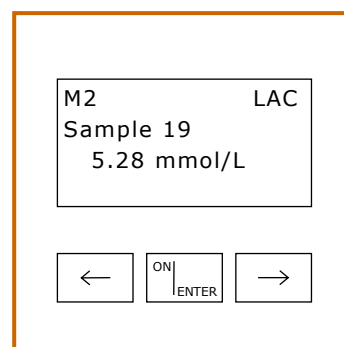

9. Insert the last cuvette, read the measured value, remove cuvette
Note: Ensure the correct order of the samples!