

Step by step instructions


GLY 742 (GLY aqu. / GLY org.)

Single measurement

Note: Before measurement, prepare the sample according to the package insert




1. Insert capillary with 10 µL sample into cuvette

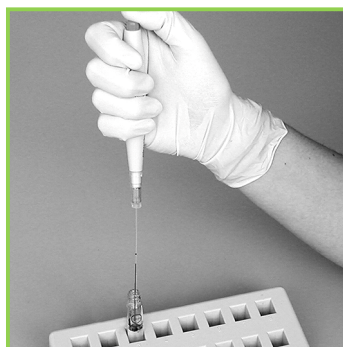


2. Eject sample several times with micropipetter into cuvette



3. Screw cap on
Turn cuvette upside down several times

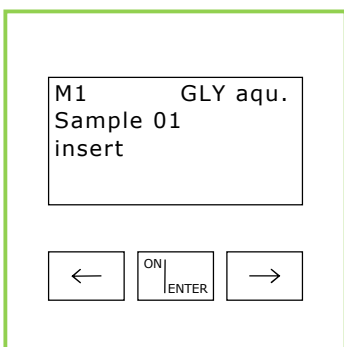

4. Switch photometer on with ON/ENTER key
Wait for device check, confirm with ON/ENTER
Select the required test, confirm with ON/ENTER

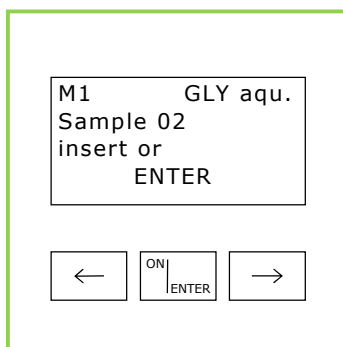


5. Zero point adjustment: Insert cuvette with sample (Fig. 3) into photometer, zero point is stored in memory
Remove cuvette after signal tone



6. Replace screw cap with starter cap



7. Turn cuvette upside down several times

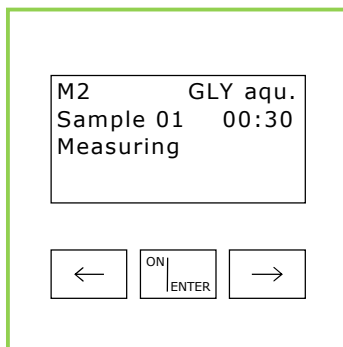

8. First press ON/ENTER
Then insert cuvette into photometer




9. Time is displayed, wait for measured value

Step by step instructions


GLY 742 (GLY aqu. / GLY org.)

Serial measurement / Number of samples per series: Up to 20 samples at the same time


Note: Before measurement, prepare the sample according to the package insert

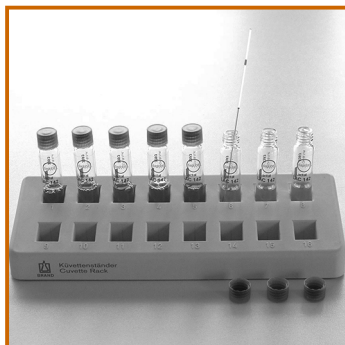


1. Eject all samples one after the other several times with micropipetter into cuvette

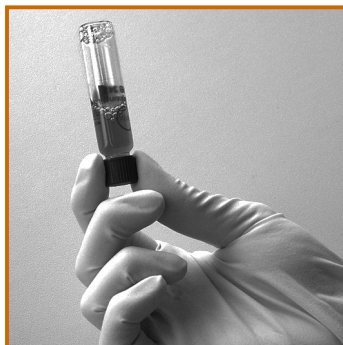

2. Screw all caps on again
Turn cuvettes upside down several times

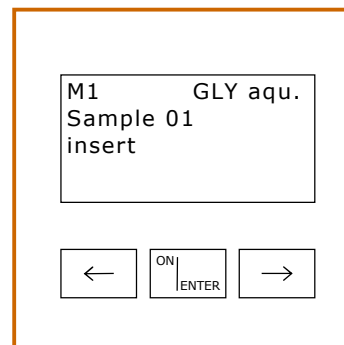

3. Switch photometer on with ON/ENTER key
Wait for device check, confirm with ON/ENTER
Select the required test, confirm with ON/ENTER

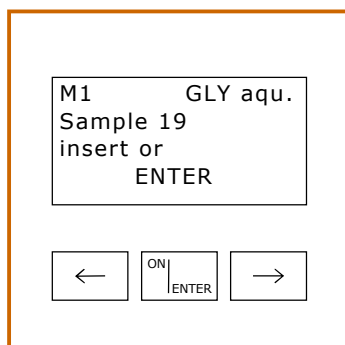

4. Zero point adjustment: Insert cuvettes with samples (Fig. 2) one after the other into photometer, all zero points are stored in memory


Note: Ensure the correct order of the samples!



5. After the zero point adjustment of the last cuvette replace all screw caps with starter caps



6. Turn all cuvettes **simultaneously** upside down, repeat several times

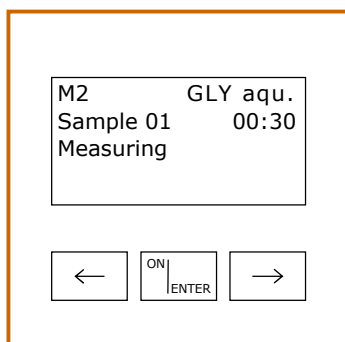


7. First press ON/ENTER key
Then insert 1st cuvette into photometer

Time is displayed, wait for measured value



8. Read the measured value of the 1st cuvette, remove cuvette

Insert 2nd cuvette, read the measured value, remove cuvette, and so on

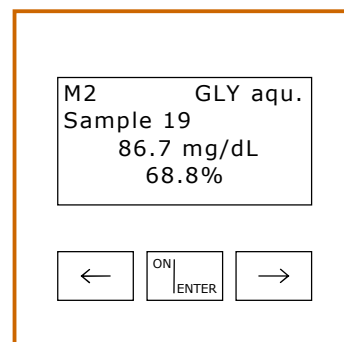

9. Insert the last cuvette, read the measured value, remove cuvette

Note: Ensure the correct order of the samples!