

Survey: **KS4/25**  
month: **May 2025**  
Participant-No: **0004965**  
valid from: **17.05.25**



page 1 of 5

diaglobal GmbH  
Dr. Rainer Schlegel  
Haus 41  
Köpenicker Str. 325  
12555 Berlin




Bonn, 10. June 2025

## Certificate

We confirm that you have participated in the survey for clinical chemical analytes in serum.  
This certificate is according to the current version of the RiliBÄK valid until the end of November 2025.

You have met the requirements of the survey for the following analytes:

cholesterol	(1)	glucose	(3)	urea	(1)
lactate	(2)	triglycerides	(2)	CK	(1)

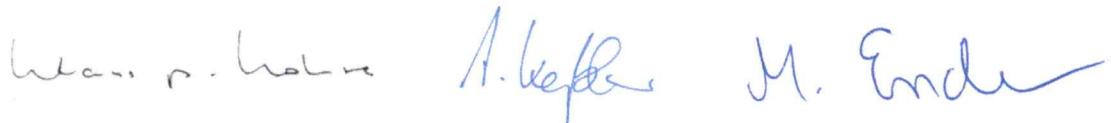

Prof. Dr. Dr. K. P. Kohse  
EQA scheme director

Dr. Anja Kessler  
Head of Reference Institute

Dr. Marika Enders  
EQAS-Board

The number in parentheses characterizes the analytical method used.  
The assignment of the number to the respective method and/or the respective instrument  
is to be taken from the total evaluation.

This certificate is valid in conjunction with the final report dated 04.06.25.  
This is available for download in the RfB-Online system.

### Listing and Evaluation of all your results

#### Explanations

#### Certificate

A certificate is issued (given) for an analyte only if the basis for an evaluation of the accuracy is given by the guidelines of the German Medical Association and/or if an evaluation is possible in analogy to these guidelines (see comments on the evaluation) and, if both results for an analyte are within the given acceptance limits. (marked as '+' below C)

#### Certificate of participation

In the participation certificate all analytes which are included in the list on this page are listed.  
If all analytes are listed on the certificate no participation certificate is printed.

Legend:	C=Certification, M=No of method, R=your result, D=difference (R-T) Dmax= maximum allowable amount of difference in measurement, partly given by annex 1 of the guideline of the BÄK. T = target value, either reference method value or assigned value, LL   UL = lower resp. upper limit	Certification:	+ = fulfilled ( quotient   D/Dmax   <= 1.0 ) - = not fulfilled (quotient   D/Dmax   > 1.0 ) ± = certification cancelled because of technical and/or analytical reasons
---------	--	----------------	---

	<b>C</b>	<b>M</b>	<b>R</b>	<b>D/Dmax</b>	<b>T</b>	<b>LL</b>	<b>UL</b>							
cholesterol [mg/dl]	+	1	A 150 B 184	0.57 0.47	139 173	120 150	158 196							
glucose [mg/dl]	+	3	A 65.9 B 80.6	-0.15 -0.26	67.4 83.9	57.2 71.3	77.6 96.5							
urea [mg/dl]	+	1	A 16.5 B 70.6	-0.54 -0.47	18.5 77.9	14.8 62.3	22.2 93.5							
lactate [mmol/l]	+	2	A 1.79 B 4.49	0.54 0.68	1.62 4.00	1.32 3.27	1.93 4.72							
triglycerides [mg/dl]	+	2	A 59.7 B 202	-0.20 0.56	61.7 185	51.8 155	71.6 215							
CK [U/l]	+	1	A 399 B 389	0.32 0.60	369 347	276 277	462 417							